

Maxpar Human Acute Myeloid Leukemia (AML) Phenotyping Panel Kit, 15 Marker—25 Tests

Catalog: 201316
 Package size: 25 tests

Storage:

- Antibodies, buffers, and water: 4 °C. Do not freeze.
- Cell-ID Intercalator-Ir: -20 °C.

Contents:

- Maxpar® Cell Staining Buffer (500 mL)
- Maxpar Fix and Perm Buffer (25 mL)
- Maxpar Water (500 mL)
- Cell-ID™ Intercalator-Ir (125 µM; 25 µL)
- Maxpar antibodies (see table for panel)*

* The antibodies are provided in individual tubes, not a premixed cocktail.

Target	Clone	Metal	Target	Clone	Metal
CD19	HIB19	142Nd	CD15	W6D3	164Dy
CD117	104D2	143Nd	CD34	581	166Er
CD11b	ICRF44	144Nd	CD3	UCHT1	170Er
CD64	10.1	146Nd	CD44	IM7	171Yb
CD7	CD7-6B7	147Sm	CD38	HIT2	172Yb
CD123	6H6	151Eu	HLA-DR	L243	174Yb
CD45	HI30	154Sm	CD184/CXCR4	12G5	175Lu
CD33	WM53	158Gd			

Technical Information

Description: The Maxpar AML Phenotyping Panel Kit is for the identification and phenotyping of human acute myeloid leukemia (AML). AML, the most common type of acute leukemia in adults, is a malignancy arising within the bone marrow due to a disruption of normal hematopoiesis. AML arises within precursors of myeloid, erythroid, megakaryocytic and monocytic cell lineages due to the acquisition of chromosomal rearrangements and multiple gene mutations. The immunophenotype of AML is highly heterogeneous; markers frequently expressed by AML include CD15, CD33, CD34 and CD64.

Recommended Usage: For staining with the Human AML Phenotyping Panel Kit, cells should be prepared using standard techniques and stained according to the [Maxpar Cell Surface Staining Protocol](#). The kit contains buffers optimized for staining and a nucleic acid intercalator used for single-cell identification. Additional materials and equipment may be required for cell staining and acquisition. Please refer to [Maxpar Cell Surface Staining Protocol](#). Data collection is performed on a CyTOF® mass cytometer.

References

Craig, F.E. and Foon, K.A. "Flow cytometric immunophenotyping for hematologic neoplasms." *Blood* 111 (2008): 3941-67.


Dick, J.E. and Lapidot, T. "Biology of normal and acute myeloid leukemia stem cells." *International Journal of Hematology* 82 (2005): 389-96.

Amir, el-AD et al. "viSNE enables visualization of high dimensional single-cell data and reveals phenotypic heterogeneity of leukemia." *Nature Biotechnology* 31 (2013): 545-52.

For technical support visit <http://techsupport.fluidigm.com>. For general support visit <http://www.fluidigm.com/support>.

For Research Use Only. Not for use in diagnostic procedures.

Information in this publication is subject to change without notice. **Safety data sheet information:** <http://www.fluidigm.com/sds>. **Patent and license information:** <http://www.fluidigm.com/legalnotices>. **Limited Use Label License:** The purchase of this product conveys to the purchaser the limited, non-transferable right to use the purchased consumable or reagent only with Fluidigm instruments and systems. **Trademarks:** Fluidigm, the Fluidigm logo, Cell-ID, CyTOF, and Maxpar are trademarks and/or registered trademarks of Fluidigm Corporation in the United States and/or other countries. © 2018 Fluidigm Corporation. All rights reserved. 08/2018

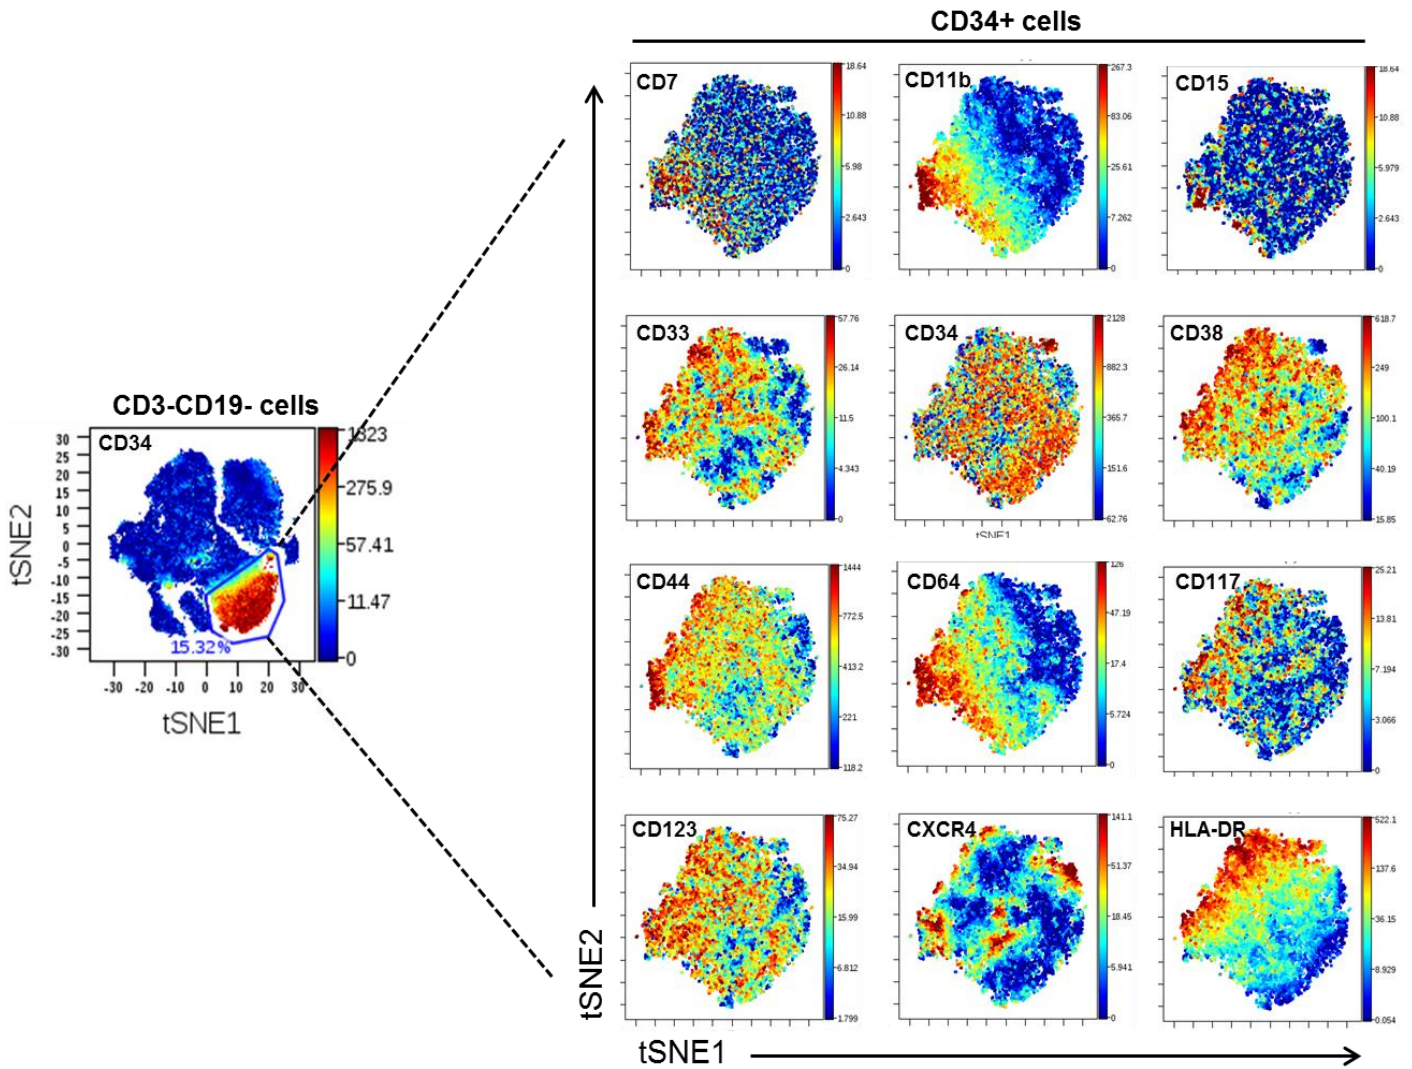

PBMC from a patient with Acute Myeloid Leukemia (AML) were stained with the Maxpar AML Phenotyping Panel Kit. The resultant data was analyzed using viSNE, which projects the multi-dimensional distance between events resolved by the markers in the panel kit into two dimensions (tSNE1 and tSNE2). The viSNE map for viable CD3-CD19- events is shown on the left, heat-mapped for CD34 expression. Further viSNE analysis of the CD34+ AML cells (right) reveals the heterogeneity within AML. Each plot is heat mapped to the indicated marker.